


00XCP-1036-01 (CPC Metal Fitting) MH3 Flowmeter with Tube

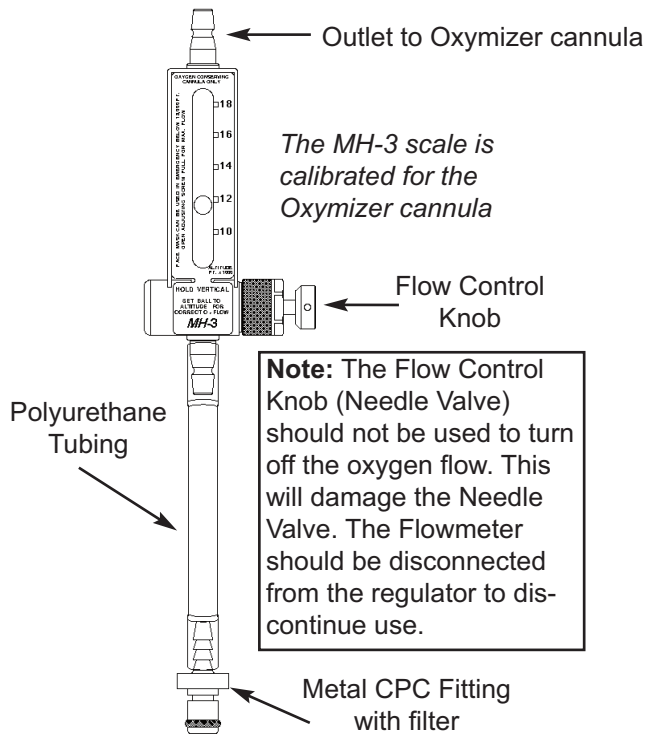

Cleaned for oxygen use per MH ESR-008


Instructions

The MH3 Flowmeter has an altitude/flow scale calibrated for the Oxymizer oxygen-conserving cannula. The scale is marked in 2,000 ft. increments for flight levels up to 18,000 ft. To receive the proper amount of oxygen, simply adjust the MH3 to where the scale reads the same altitude you are flying. Example: If you are at 15,000 ft. you would hold the flowmeter vertical and adjust the needle valve on the MH3 to where the ball reads between the 14 and 16 scale. Counter clock-wise increases and clock-wise decreases the oxygen flow. The outlet flow of the MH3 can be adjusted well beyond the limits of the scale for emergency purposes. You can operate the XCP system at flight levels above 18,000 ft. with the MH4 flowmeter and XCP facemask. This will however, use much more oxygen.



5IXCP-1036-01\$-1
2020-M-D TBD

00XCP-1036-01 (CPC Metal Fitting) MH3 Flowmeter with Tube

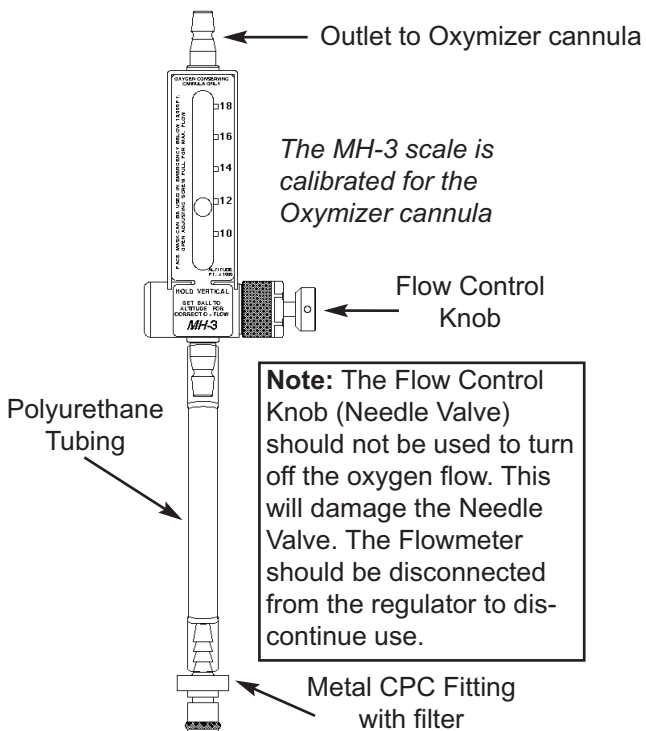


Cleaned for oxygen use per MH ESR-008

Instructions

The MH3 Flowmeter has an altitude/flow scale calibrated for the Oxymizer oxygen-conserving cannula. The scale is marked in 2,000 ft. increments for flight levels up to 18,000 ft. To receive the proper amount of oxygen, simply adjust the MH3 to where the scale reads the same altitude you are flying. Example: If you are at 15,000 ft. you would hold the flowmeter vertical and adjust the needle valve on the MH3 to where the ball reads between the 14 and 16 scale. Counter clock-wise increases and clock-wise decreases the oxygen flow. The outlet flow of the MH3 can be adjusted well beyond the limits of the scale for emergency purposes. You can operate the XCP system at flight levels above 18,000 ft. with the MH4 flowmeter and XCP facemask. This will however, use much more oxygen.



5IXCP-1036-01\$-1
2020-M-D TBD

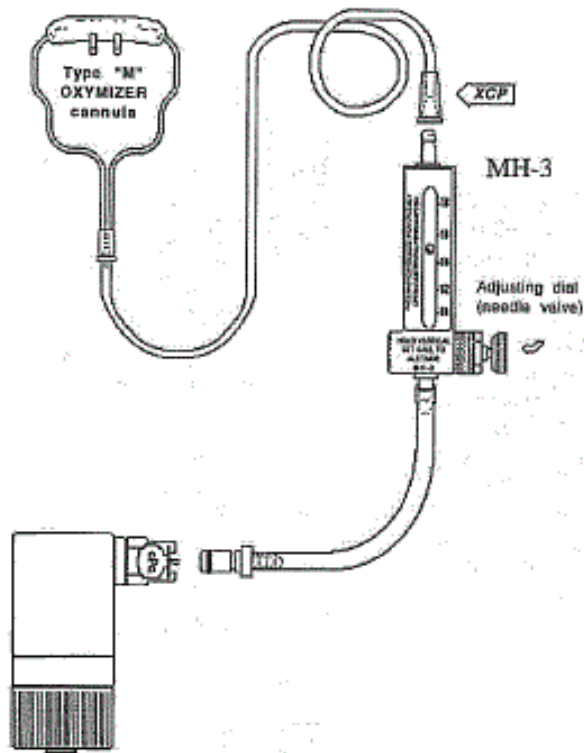


XCP MH3 flowmeter/regulator reference & quick-start instructions

Make sure that the inlet bushing on the cannula is securely on the flowmeter. It can be removed and reconnected many times over.


To insert:

Simply insert the male connector into the female connector on the XCP regulator. Push in to yield a definite "click" sound. You will now have a positive and air-tight connection where the mechanically activated check valve will open to allow oxygen to flow.

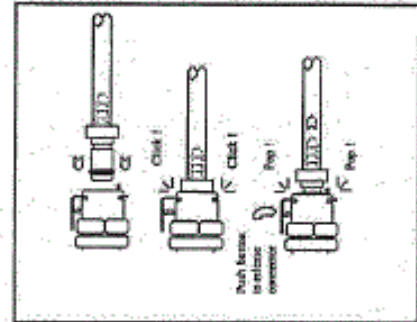

To remove:

With your thumb or finger simply push the side release button in. The male connector will "pop" out and the mechanically activated check valve will snap back shut.

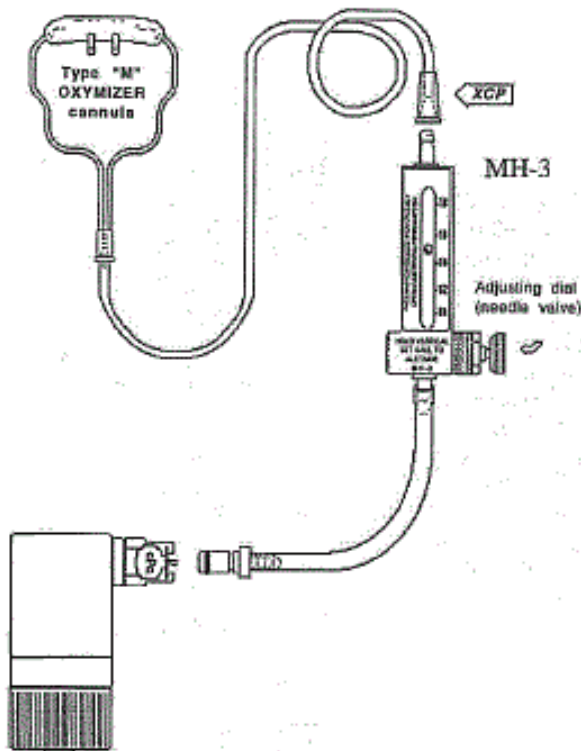


XCP MH3 flowmeter/regulator reference & quick-start instructions

Make sure that the inlet bushing on the cannula is securely on the flowmeter. It can be removed and reconnected many times over.

To insert:

Simply insert the male connector into the female connector on the XCP regulator. Push in to yield a definite "click" sound. You will now have a positive and air-tight connection where the mechanically activated check valve will open to allow oxygen to flow.

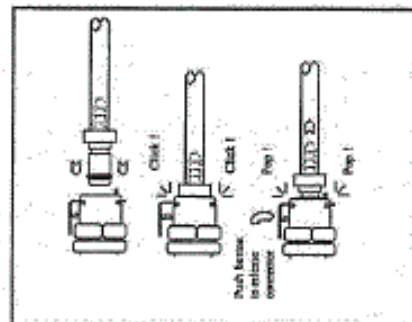

To remove:

With your thumb or finger simply push the side release button in. The male connector will "pop" out and the mechanically activated check valve will snap back shut.